


Healthcare Device Standards

- Roadmap perspectives
- Workshop

A number of standards activities and related artifact developments are involved in the harmonization process.

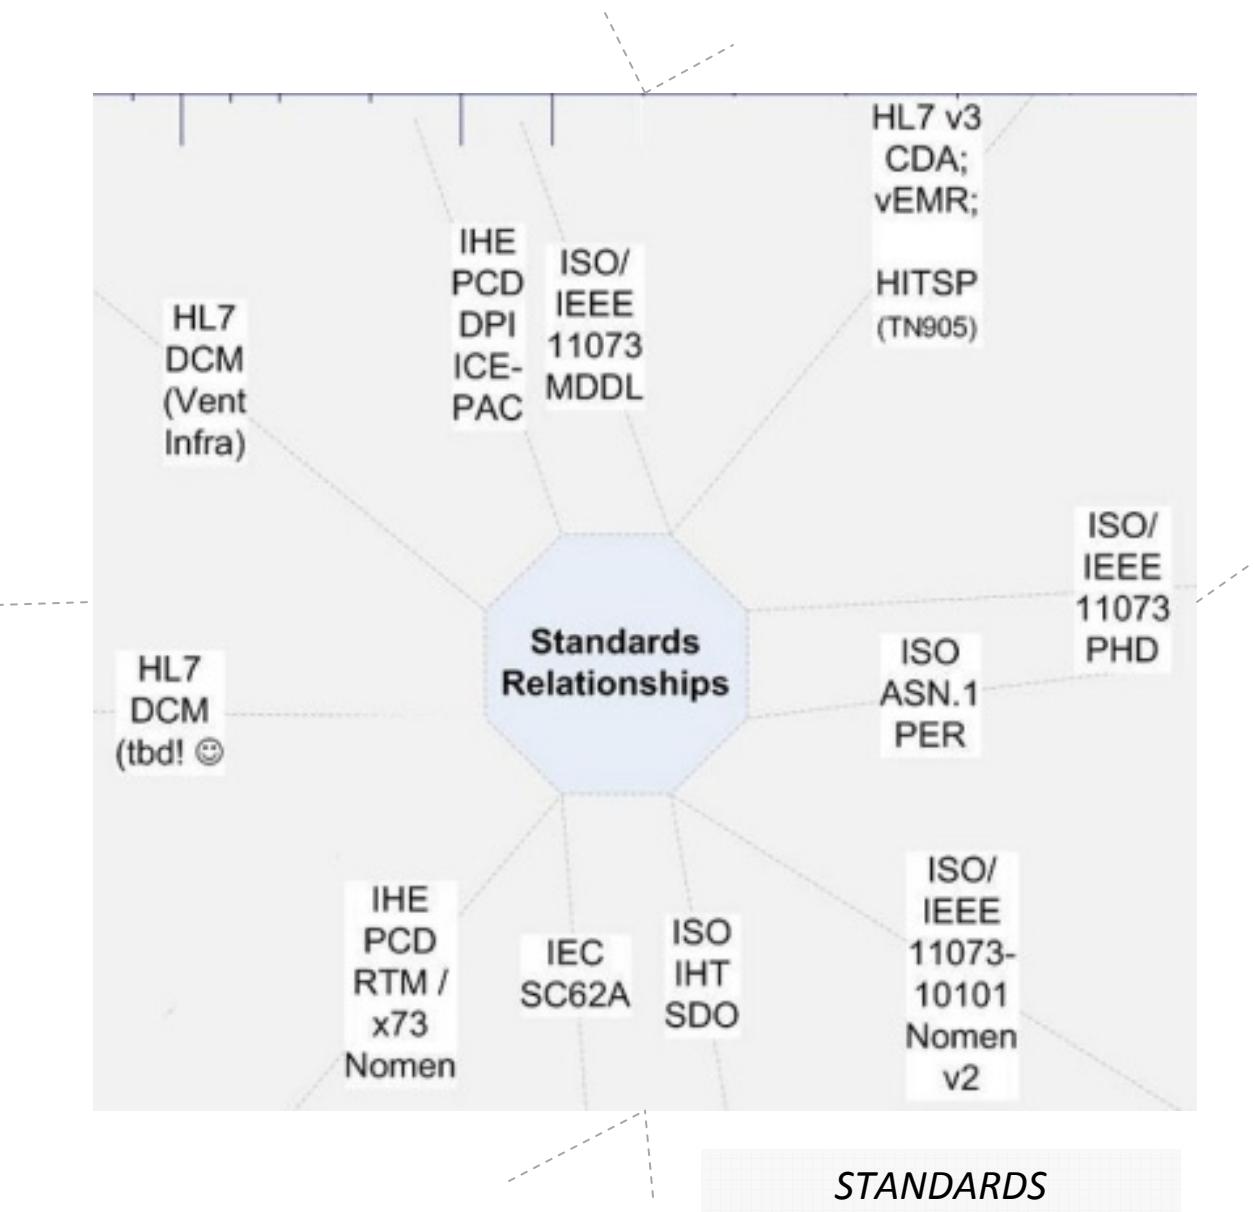

CDS

CLINICAL
MODALITY

PERSONAL
MODALITY

VENTILATED PT. TRF

PACU

INTERM


ICU

VENT

VENT

VENT

Other
e.g. Oxy-
Vent
Optimzn

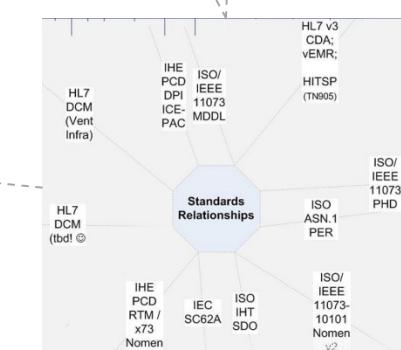

STANDARDS

SEM. ARCH.
ONTOLOGY

VENT

PUMP

VS

...

IDC

aECG

NOMENCLATURE

COMM FACIL

CDS



DCM



IHE PCD et al

CLINICAL MODALITY

PERSONAL MODALITY

VENTILATED PT. TRF

PACU

INTERM

ICU


VENT

VENT

VENT

DCM/DPI RDC

Other
e.g.Oxy-
Vent
Optimzn



ICSG/MDIB

PHD

SEM. ARCH. ONTOLOGY



DB

VENT

PUMP

VS

...

PHD



RTMMS

IDC

aECG

NOMENCLATURE

COMM FACIL

CDS



DCM



IHE PCD et al

CLINICAL
MODALITY

PERSONAL
MODALITY

VENTILATED PT. TRF

PACU

INTERM

ICU

VENT

VENT

VENT

DCM/DPI RDC

Other
e.g.Oxy-
Vent
Optimzn



ICSG/MDIB

PHD

SEM. ARCH.
ONTOLOGY



DB

VENT

PUMP

VS

...

PHD

IDC

aECG

NOMENCLATURE


RTMMS

COMM EACH

- Deployment topology

- Quality system

Clinical patient care system encompasses a range of distributed, synergistic workgroups.

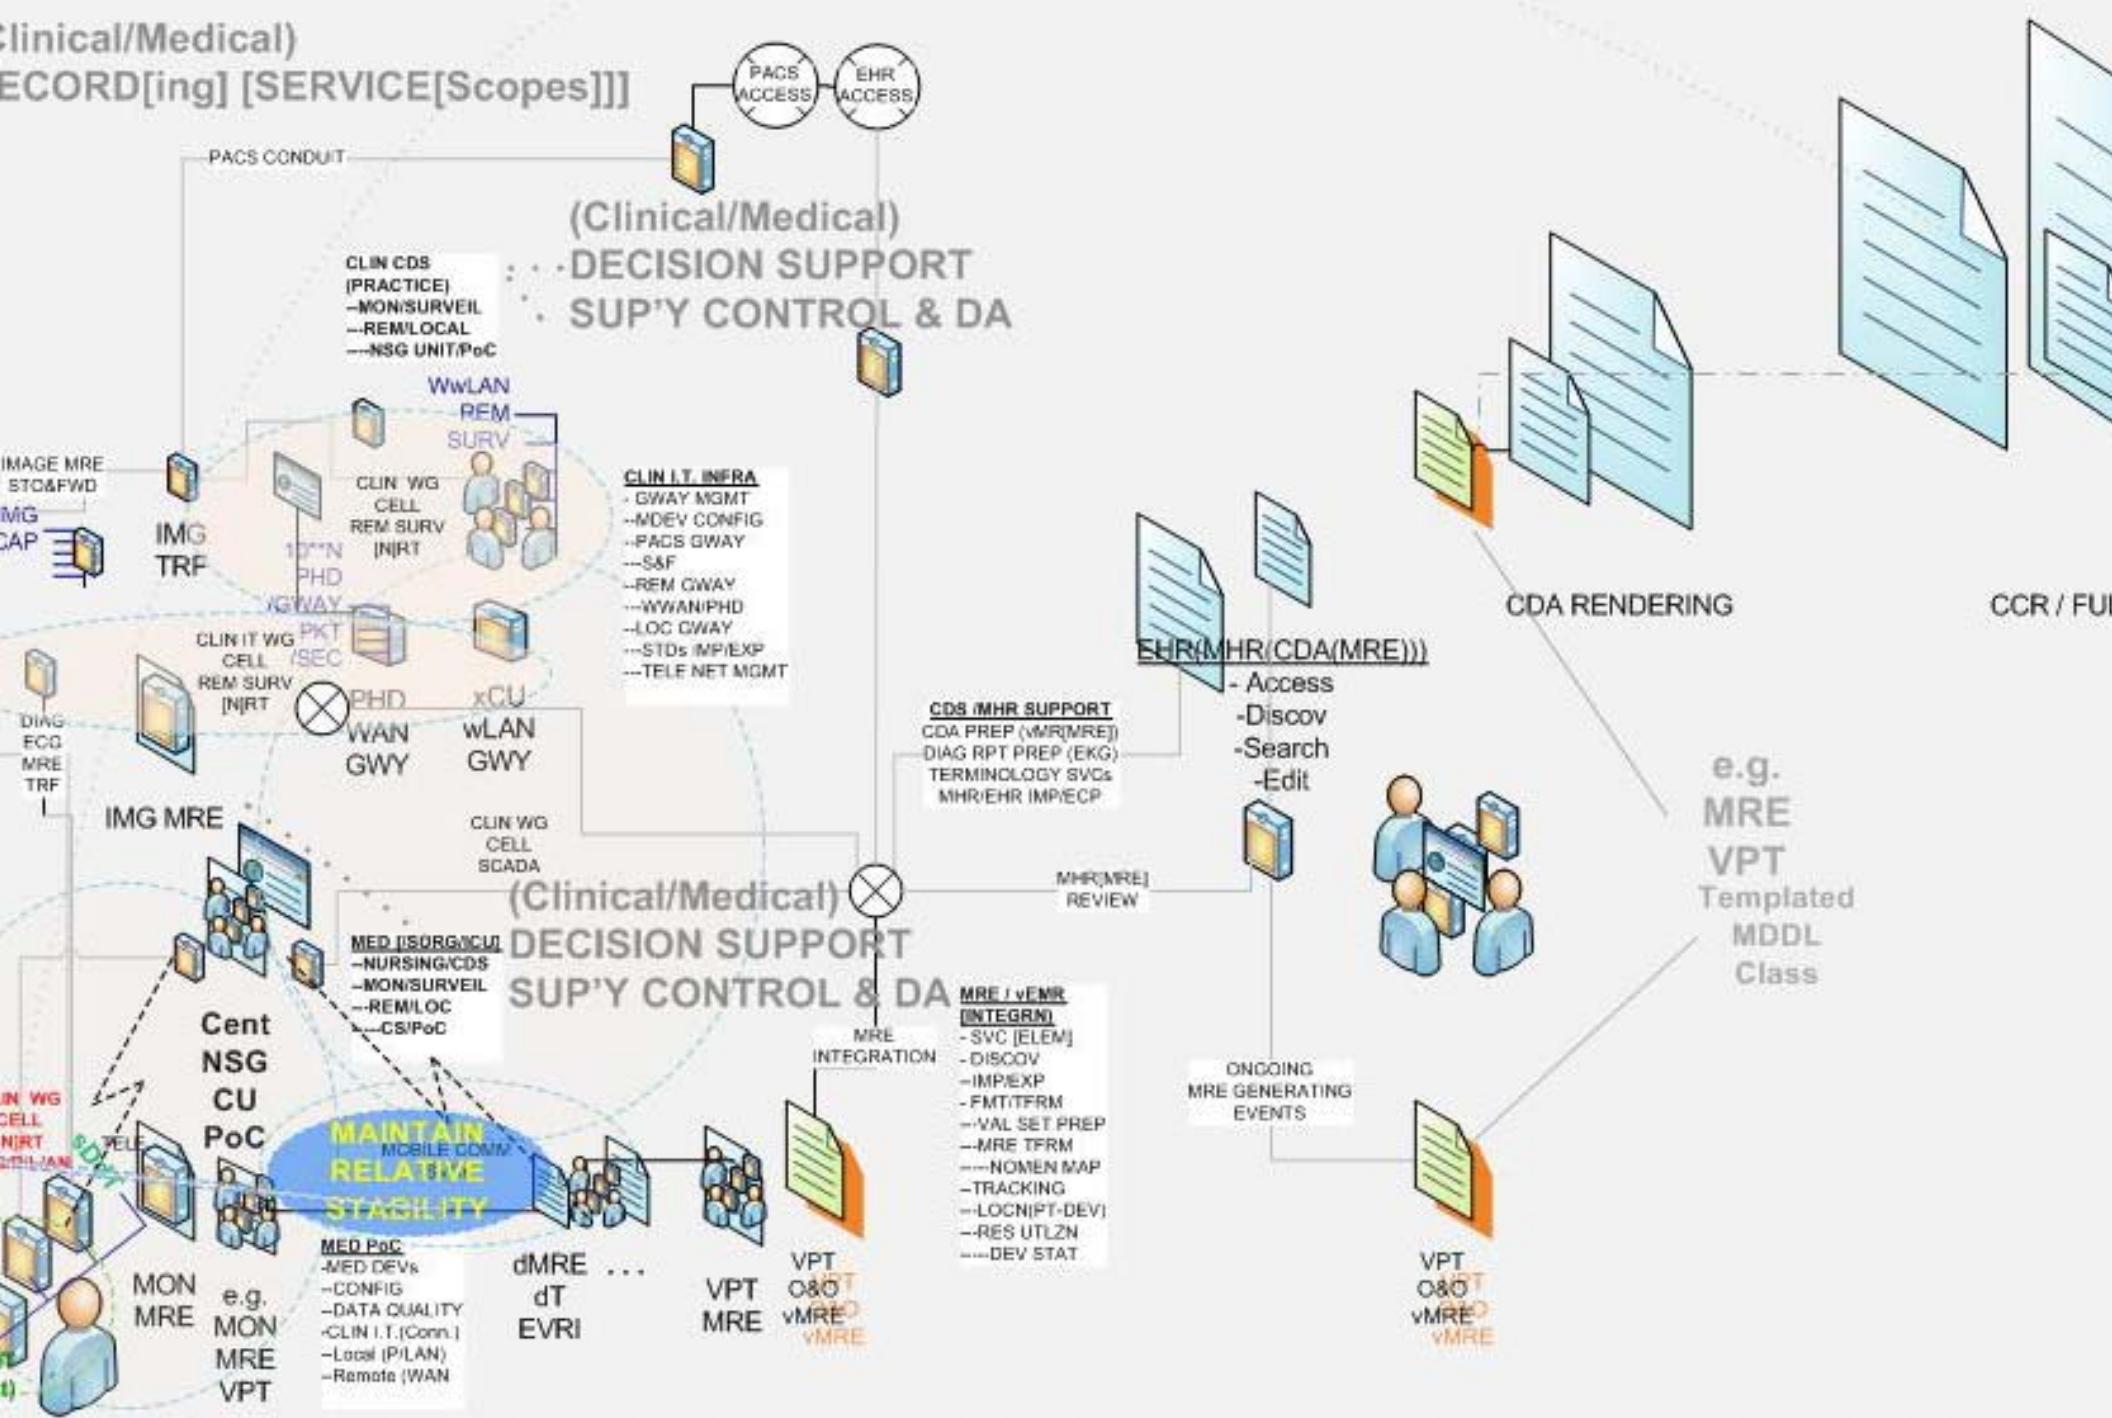

quality system" encompasses regulatory, vendor, and [end-]user workgroups/systems.

